


CERTIFIED COPY (CPLR RULE 4518)

0.10% SIMULATOR SOLUTION RECORD

Lot Number 21390, dated October 5, 2021

I, Jennifer F Limoges, Associate Director of Forensic Science, Forensic Investigation Center, do hereby certify and authenticate, as provided by Rule 4518, subdivisions a and c, Civil Practice Law and Rules, that the document annexed hereto is a true and accurate representation of an electronic record of the New York State Police Forensic Investigation Center which has been delegated to my possession, custody and control by the Superintendent of the New York State Police. This record, once created, is stored in an electronic format that cannot, thereafter, be altered or modified. This record was made in the regular course of business of the New York State Police Forensic Investigation Center, it is the regular course of the Forensic Investigation Center business to make such record, and such record was made at the time of each event recorded in it or within a reasonable time thereafter.

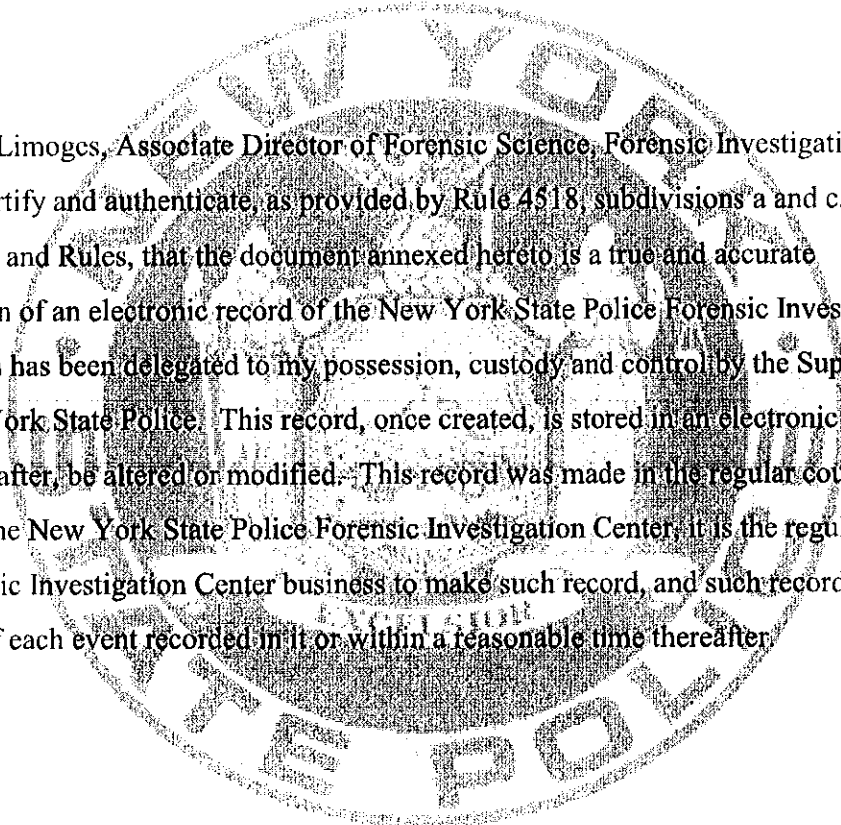

Jennifer F. Limoges

Digitally signed under
ESRA by Jennifer F
Limoges on
2021.10.19 06:59:54 -04'00'

Jennifer F Limoges
Associate Director of Forensic Science
Forensic Investigation Center



**State
Police**

**Forensic
Investigation
Center**

KATHY HOCHUL
Governor

KEVIN P. BRUEN
Superintendent

DR. RAY A. WICKENHEISER
Director

0.10% SIMULATOR SOLUTION RECORD

Report Date: October 5, 2021
Manufacturer: Guth Laboratories, Inc.
Lot Number: 21390
Expiration Date: 3/22/2022
Analysis Results: 123 mg Ethyl Alcohol / 100 mL of solution

I, Carol S Miller, D-ABFT-FA, tested simulator solution lot number 21390 by headspace gas chromatography and have determined that it contains the appropriate concentration of ethyl alcohol. This solution is hereby approved for use.

When this simulator solution is used with a properly operating breath testing instrument, it will provide a value of 0.10% within acceptable limits.

I, Carol S Miller, D-ABFT-FA, made the entries contained in this record at the time of each event recorded, or within a reasonable time thereafter.

Performed by:

Reviewed by:

Digitally signed under
ESRA by Carol S Miller on
2021.10.05 11:44:00 -04'00'

Digitally signed under ESRA
by Carrie A Kirkton on
2021.10.18 09:33:25 -04'00'

Carol S Miller, D-ABFT-FA
Forensic Scientist III

Breath Analysis Technical Supervisor/Operator #43419

Carrie A Kirkton, D-ABFT-FA

Supervisor of Forensic Services

Breath Analysis Technical Supervisor